



PCBPTIP replacement instructions

Replacement tip for boroscopic probes, PCBP series

! Make sure to perform this procedure in a clean, non-dusty environment in order to prevent dust or other particles from entering the lens.

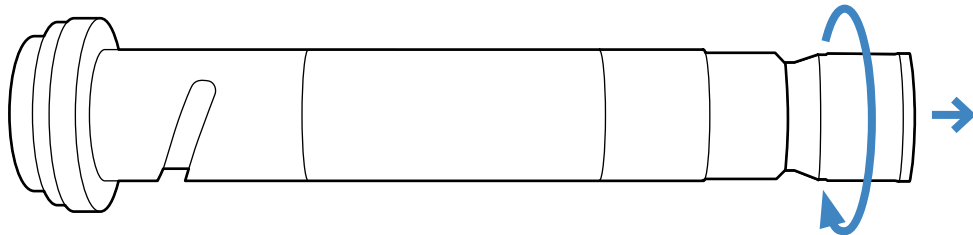

- 1 Unscrew the optical tip of the probe to remove it

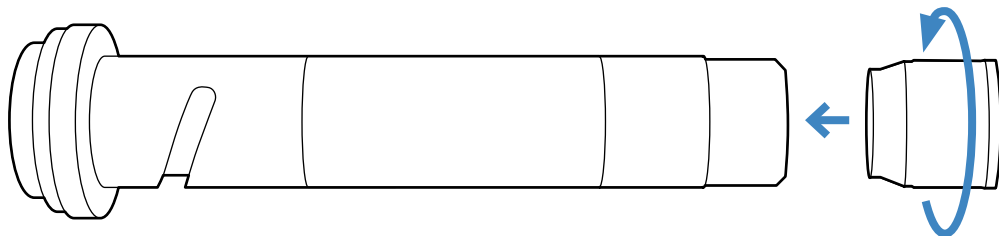

- 2 Insert new PCBPTIP replacement